

PRE-TREATMENT REPORT

Clinic: RadOnc UChicago Medicine
5758 S Maryland Avenue
Chicago IL 60637

Plan: 1-2 RUL
Planned: 05.09.2019 2:26 PM jpartouche
Measured: 05.09.2019 7:05 PM planning
Accepted: 05.09.2019 7:15 PM planning
Comments:


Treatment Summary

Radiation Device: TrueBeam1
Temperature: 22.5 °C
Reference: Planned Dose

Beam	Gantry	Energy	Daily corr factor	Norm dose	Det within acceptance Dev	DTA	γ-index	Median dose dev
Composite				1151 cGy	94.7%	99.6%	99.5%	-1.0%
04 CCW	21° to 181°	6 MV, FFF.010		432 cGy	95.4%	99.6%	100.0%	-0.6%
05 CW	181° to 21°	6 MV, FFF.010		402 cGy	94.9%	98.3%	100.0%	-1.3%
06 CCW	21° to 181°	6 MV, FFF.010		426 cGy	90.2%	99.6%	100.0%	-1.0%

Histograms

Reference: Planned dose

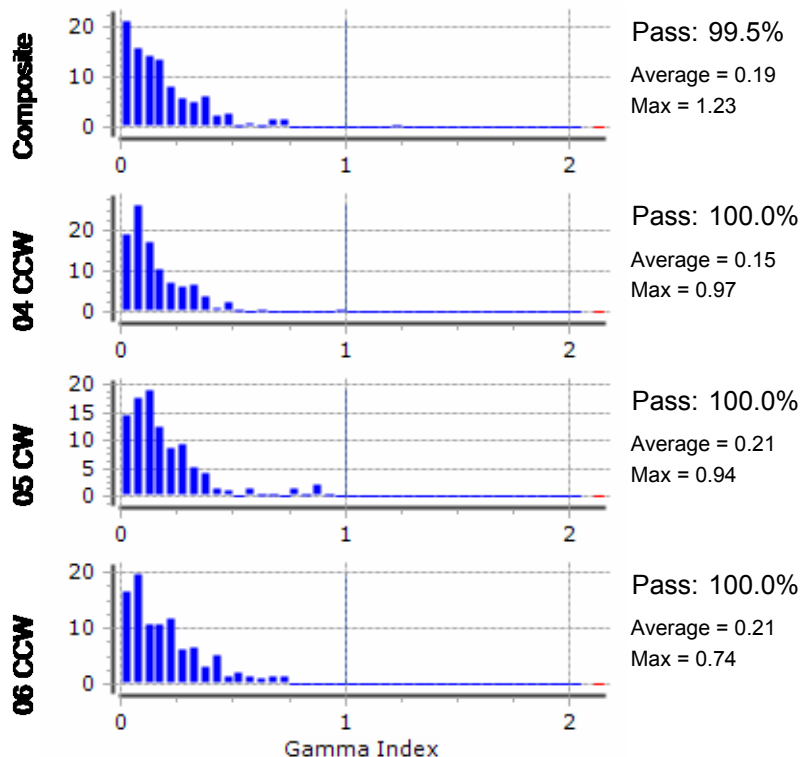

PRE-TREATMENT REPORT





Parameter Definitions & Acceptance Criteria, Detectors

Parameter	Selected Detectors	Δ Dose	Δ Dist	Acceptance Limits
Dose Deviation	Dose from 10% to 500%	n.a.	n.a.	90% within $\pm 5.0\%$
Dist to Agreement	Gradient $\geq 1\%/mm$	n.a.	n.a.	90% with DTA ≤ 3.0 mm
Gamma Index	Dose from 10% to 500%	$\pm 3.0\%$	3.0 mm	95% with gamma ≤ 1

PRE-TREATMENT REPORT



Absolute dose, Composite

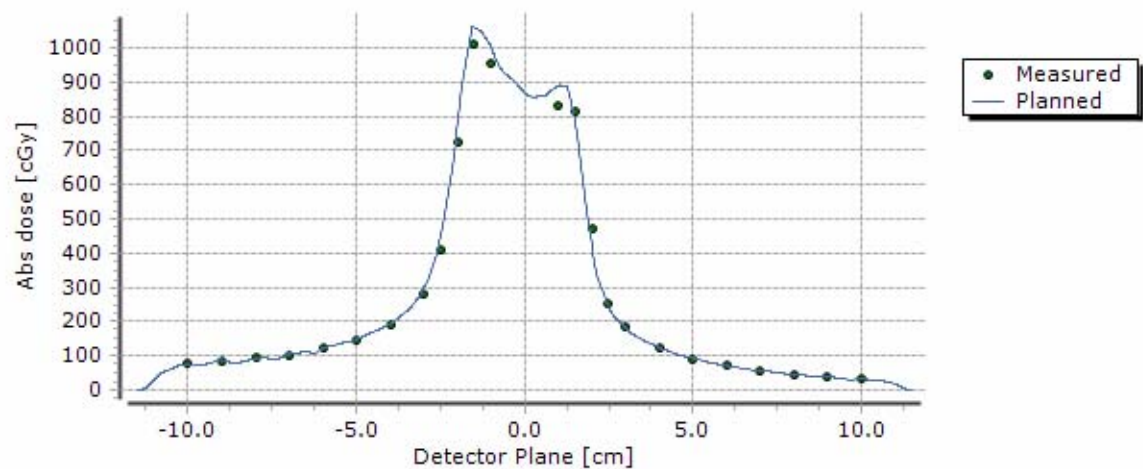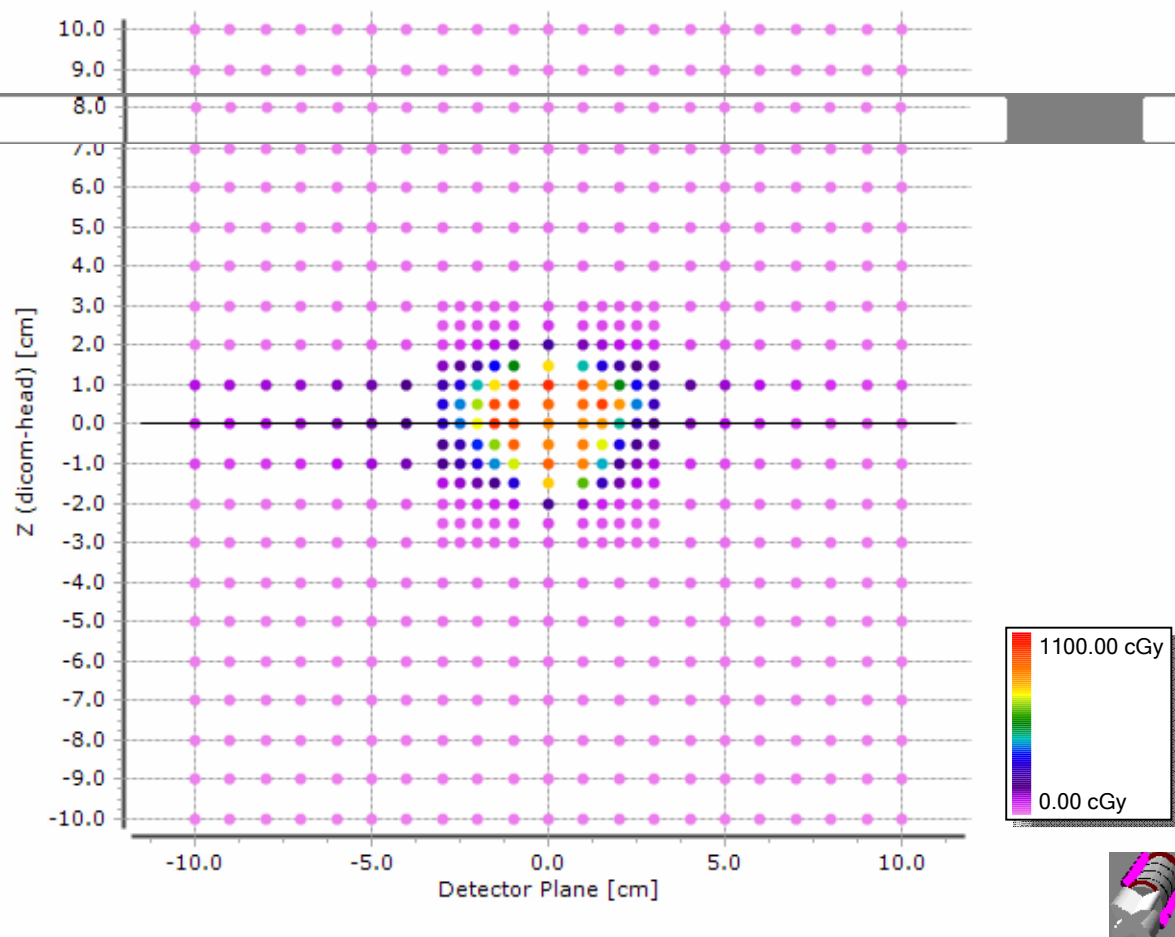

PRE-TREATMENT REPORT



Absolute dose, Composite

